Lab 6 Lab Techniques

Samer Alqaraleh,

PhD. Nanobiotechnology


Faculty of Medicine, Mutah university

Immunology, 2nd year students

1. Flow Cytometry

- The term 'cytometry' is defined as a measurement of the physico-chemical properties of cells. 'Flow cytometry' is the measurement of cells and other particles in a flow.
- Can analyze the <u>cell surface</u> or <u>intracellular expression</u> of different molecules.
- The <u>maturation stage</u>, <u>cytokine secretion</u> (inside cells and bound) or <u>cell cycle</u>, <u>apoptotic</u> cell and <u>numerating</u> B, T, and other leukocyte cells.
- The flow cytometer is a specialized instrument that can detect fluorescence on individual cells in a suspension and thereby determine the number of cells expressing the molecule.


- Cytoplasmic molecules can be stained by temporarily permeabilizing cells and permitting the labeled antibodies to enter through the plasma membrane.
- lipophilic Fluorescent dyes can be used to study the proliferation of T and B cells in vivo. One commonly used dye of this type is **CarboxyFluoroscein Succinimidyl Ester (CFSE)**.
- Flow cytometers also <u>identify</u> and <u>separate</u> the cells depending on the cell <u>size</u> and <u>internal complexity</u> by forward (size) and side light-scattering (complexity) properties of cells.
- This information is often used to distinguish different cell types. For example, neutrophils and monocytes.

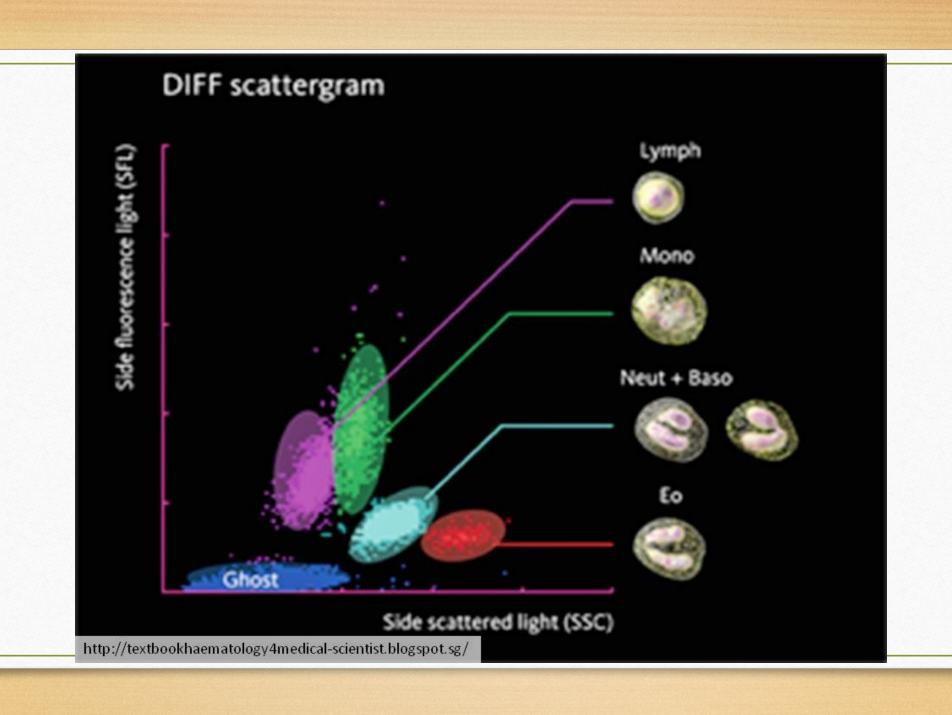

- Once a cell/object comes into the path of a ray of light (Laser), the light changes its orientation. This phenomenon is called light scatter and occurs under all angles between 0 and 360°.
- Detection of this scattered light provides information on the size and the quality of the object.

2. A. Ag-Ab binding affinity

- A method, more commonly used today, to measure the kinetics of antigen-antibody interactions depends on **Surface Plasmon Resonance**.
- In this method, an antibody passed over an antigen that is fixed over a metal film. A light source is focused on this film before passing antibody through a prism at a specific angle (resonance), and the reflected light provides a surface plasmon resonance readout. Adsorption of an antibody to the antigen alters the surface plasmon resonance readout, and this alteration makes an angular shift and as it increase means increase antibody affinity.

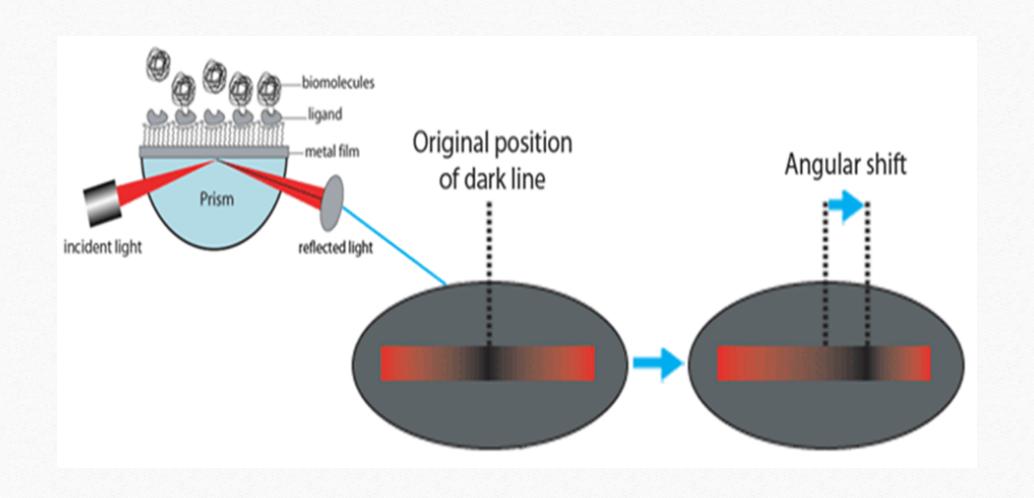


B. Equilibrium dialysis

- Antibody affinities for antigen can be measured directly for small antigens (e.g., haptens) by a method called **equilibrium dialysis**.
- In this method, the antigen with radioactive material in the bathing solution enters until the concentration of antigen within the two membrane-side (semi-permeable for antigen) compartments becomes exactly the same (the same radioactivity)).
- A solution of antibody is confined in one compartment. when antibody is present in one compartment, the net amount of antigen inside the antibody compartment increases and the radioactivity increases by the quantity that is depending on antibody affinity.

1. Strength of Ag-Ab Interactions

Control: No antibody present (ligand equilibrates on both sides equally)

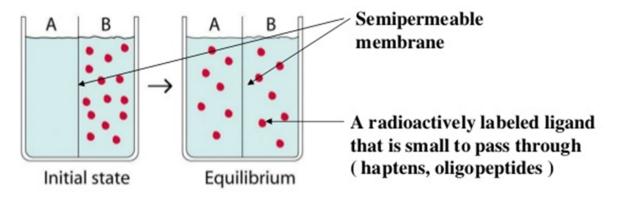

Experimental: Antibody in A (at equilibrium more ligand in A due to Ab binding)

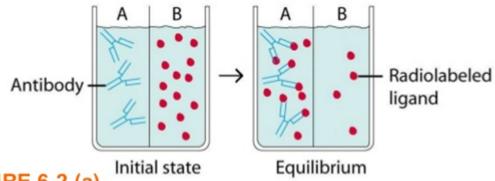


FIGURE 6-2 (a)

Determination of Ab affinity (Ka) by equilibrium dialysis.

Immunohematology

• The term **immunohematology** refers to the <u>serologic</u>, <u>genetic</u>, <u>biochemical</u>, and <u>molecular</u> study of antigens associated with membrane structures on the blood cells, as well as the <u>immunologic properties</u> and <u>reactions</u> of blood components and constituents.

- Transfusion medicine is a multidisciplinary specialty encompassing all aspects of:
- ✓ blood donation.
- ✓ blood component preparation.
- ✓blood cell serology.
- ✓ blood transfusion therapy.

 Operationally, transfusion medicine is divided between blood centers and transfusion services.

- **Blood centers** recruit and collect blood from donors and manufacture and distribute blood components.
- Transfusion services perform pretransfusion compatibility testing (blood grouping and cross match), select and issue blood components for patients, and provide medical support for blood transfusion.

Blood bank

- Units of WB and packed RBC are both kept refrigerated at 33.8 to 42.8 °F (1.0 to 6.0 °C), with maximum permitted storage periods of 35 and 42 days respectively.
- When keeping blood tube in standing position, a layer between the red cells and the plasma is formed and referred to as the **buffy coat** and is sometimes removed to make platelets and WBC for transfusion.
- Platelets have a shelf life of 5 to 7 days. Platelets are stored at room temperature (72 °F or 22 °C) and must be rocked/agitated

• If the plasma is frozen promptly and is intended for transfusion, it is typically labeled as <u>fresh frozen plasma</u>. If it is intended to be made into other products, it is typically labeled as recovered plasma or plasma for fractionation.

Blood test tubes or Vacutainers



Order of Draw	Tube Stopper Color	Additive	Dept.	Tests	Liquid Part post centrifugation
1	Yellow 🔚	Sodium polyethanol sulfonate (SPS)	Microbiology	Blood Culture	Plasma
2	Light Blue	Sodium Citrate	Coagulation	PT, PTT	Plasma
3	Red (plain)	No additive	Tube Blood Bank	Type, RH, antibody screen, type & crossmatch	Serum
4	Red & Grey or	Clot Activator	Routine Chemistry	All STAT tests + Iron, folate	Serum
5	Green	Heparin	STAT Chemistry	BMP, CMP, Glucose, K, Troponin, Bilirubin	Plasma
6	Lavender 📗	K2EDTA	Hematology	CBC, ESR	Plasma
7	Pink	EDTA	Gel Blood Bank	Type, RH, antibody screen, type & crossmatch	Plasma
8	Gray C	Sodium Flouride (inhibits glycolysis)	Chemistry	Lactic Acid, Gluc (not run right away)	Plasma

Plasma VS Serum EDTA tube (purple) Plain tube (Red)

